

Catalog Number AS 013 RB

Highlights:

- Results in 10 minutes or less
- Available as 100-strip kits

Contents of Kit:

- 100 QuickStix Strips packed in two moisture-resistant canisters
- 100 extraction vials
- EB2 Buffer

Items Not Provided:

- Proctor Silex® Fresh Grind™ Model E160B Coffee Grinder or equivalent*
- Weigh boats* or weigh paper
- Pipette capable of delivering between 1 and 3 mL of buffer*

* Available through Envilab as accessory items; see list on page 3



Weigh, grind seeds



Transfer seeds to vial

Intended Use

This EnviroLogix QuickStix Kit for LibertyLink Rice is designed to extract and detect PAT/bar protein in bulk rice samples. The QuickStix Strips will detect 1.33% Event LL601 rice (i.e. 1 LL601 seed in 75 non-transgenic seeds). Testing multiple 75-seed samples makes it possible to detect 1% or 0.5% contamination with increasing confidence levels. This kit will also detect PAT/bar expressed by other types of LibertyLink rice; since the protein is the same, differentiation between them may be confirmed by alternate methods.

How the Test Works

In order to detect the PAT/bar protein expressed by LibertyLink rice, the sample must first be extracted in buffer to solubilize the protein. Each QuickStix strip has an absorbent pad at each end. The protective tape with the arrow indicates the end of the strip to insert into the reaction vial. The sample will travel up the membrane strip and be absorbed into the larger pad at the top of the strip. The portion of the strip between the protective tape and the absorbent pad at the top of the strip is used to view the reactions as described under “Interpreting the Results”. Please avoid bending the strips.

Selecting a Sampling Protocol

The sampling scheme can dramatically affect the probabilities and level of confidence in detecting any LibertyLink rice that may be commingled in the sample. The chart that follows shows the probability of detecting a given concentration of LL601 rice in the sample, and how the probability of detection is increased with multiple samples.

Table 1 – Number of 75-seed subsamples required

Confidence Level	LL601 Screening Level			
	5%	3%	1%	0.5%
95%	1	1	4	8
99%	1	2	7	13

Sample Preparation

This protocol calls for a small sample to be analyzed. It is essential that this sample be well-mixed and representative of the larger bulk. It is the responsibility of the user to ensure proper sampling and thorough mixing prior to analysis. The USDA has published recommended guidelines for obtaining representative grain samples (see list of references on page 3). Once representative samples have been obtained from the truck or container, they can be reduced in size using a splitter and uniformly ground and mixed using a coffee grinder or equivalent.


1. Weigh sample and add to the grinder. Either count 75 seeds and weigh, or determine average weight of seeds to be tested [weigh 100 seeds, divide by 100]; calculate the weight of the sample to be tested [number of seeds x average weight/seed].
2. Grind sample for 60 seconds until all whole grains are finely ground. Empty ground rice in a weigh boat or weigh paper, then carefully transfer to the 5 mL Extraction Vial.



Add buffer, cap and shake



Place strip in extraction vial

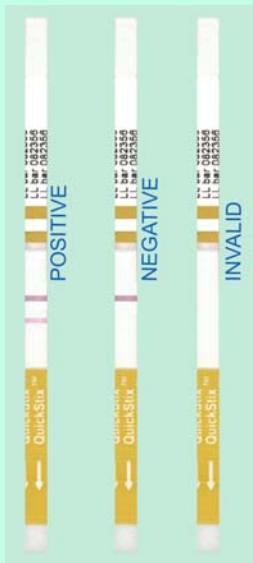

Any clearly discernable pink Test Line is positive



3. Calculate 1.5 times the weight of the sample to determine the volume of buffer. (For example, 75 seeds with a total weight of 1.5 grams would require 2.25 mL buffer.) Use a pipette to accurately add buffer to the vial, then cap and shake for 30 seconds. Allow the extract to settle for about 1 minute to create a pool of extract on top of the grain bed. No further transfer is required; the test will run in the Extraction Vial.

Important: To prevent cross-contamination, thoroughly clean grinder parts to remove dust and residue prior to preparation of each sample. Use a new vial for each sample. Do not re-use pipette tips or disposable pipettes.

How to Run the QuickStix Strip Test


1. Allow refrigerated canisters to come to room temperature before opening. Remove the QuickStix Strips to be used. Avoid bending the strips. Reseal the canister immediately.
2. Place the strip into the extraction vial. Don't push strip into settled solids. The liquid sample will travel up the strip.
3. Allow the strip to develop for 10 minutes before making final assay interpretations. Positive sample results may become obvious much more quickly.
4. To retain the strip, cut off and discard the bottom section of the strip covered by the arrow tape.

Interpreting the Results

Development of the Control Line within 10 minutes indicates that the strip has functioned properly. Any strip that does not develop a Control Line should be discarded and the sample re-tested using another strip.

If the sample extract contains PAT/*bar*, a second line (Test Line) will develop on the membrane strip between the Control Line and the protective arrow tape. Any Test Line, no matter how light, should be interpreted as positive for LibertyLink expression.

If no Test Line is observed after 10 minutes, the results should be interpreted as negative. A negative result means the sample contains less than 1.33% LibertyLink rice.

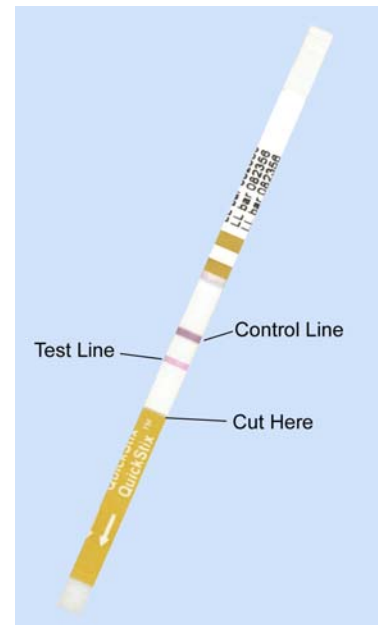

Kit Storage

QuickStix can be stored at room temperature, or refrigerated for a longer shelf life. Note the shelf life on the kit box for each storage temperature. The kit may be used in field applications; however, prolonged exposure to high temperatures may adversely affect the test results. Do not open the desiccated canister until ready to use the test strips.

USDA Resources:

<http://www.archive.gipsa.usda.gov/reference-library/handbooks/grain-insp/grbook1/bk1.pdf> - USDA Grain Inspection Handbook, Book 1, Grain Sampling.

<http://www.archive.gipsa.usda.gov/biotech/sample2.htm> - Guidance document entitled Sampling for the Detection of Biotech Grains.

<http://www.archive.gipsa.usda.gov/biotech/sample1.htm> - Practical Application of Sampling for the Detection of Biotech Grains.

<http://www.archive.gipsa.usda.gov/biotech/samplingplan1.xls> - This website provides a simple to use Sample Planner (29K Excel Spreadsheet). The planner allows you to enter different assumptions in terms of sample size, number of samples, acceptable quality level and to determine the probability of accepting lots with given concentration levels. It also plots the probabilities in graph form for easy interpretation. Specific data can be saved for documentation and future analyses.



Precautions and Limitations

- This kit is designed for screening for presence or absence only and is not meant to be quantitative.
- As with all tests, it is recommended that results be confirmed by an alternate method when necessary.
- The assay has been optimized to be used with the protocol provided in the kit. Deviation from this protocol may invalidate the results of the test.
- The results generated through the proper use of this kit reflect the condition of the working sample directly tested. Extrapolation as to the condition of the originating lot from which the working sample was derived should be based on sound sampling procedures and statistical calculations which address random sampling effects, non-random seed lot sampling effects, and assay system uncertainty. A negative result obtained when properly testing the working sample does not necessarily mean the originating lot is entirely negative for the analyte or protein in question.
- A negative result with this kit does not mean that the sampled grain has not been otherwise genetically modified.
- A strong positive result may safely be interpreted in as little as 5 minutes after sample addition. It is not safe, however, to conclude that a sample is negative before a full 10 minutes has elapsed. A weakly positive sample may require the full 10 minutes for a distinct Test Line to appear.
- Protect all components from hot or cold extremes of temperature when not in use. Do not leave in direct sunlight or in vehicle.

Optional Items Available

- Proctor Silex Fresh Grind Model E160B Coffee Grinder (ACC 040)
- Weigh boats (100/pk, ACC 047)
- Pipette and bulb (ACC 048 [5 mL pipette], ACC 049 [bulb])



**For Technical Support
Contact Us At:**

Envilab GmbH
Cyriakusstraße 27

47839 Krefeld

Tel: (02151) 5671549

Fax: (02151) 5695602

e-mail:
info@envilab-gmbh.de

website:
www.envilab-gmbh.de



LIMITED WARRANTY

EnviroLogix Inc. (“EnviroLogix”) warrants the products sold hereunder (“the Products”) against defects in materials and workmanship when used in accordance with the applicable instructions for a period not to extend beyond a product’s printed expiration date. If the Products do not conform to this Limited Warranty and the customer notifies EnviroLogix in writing of such defects during the warranty period, including an offer by the customer to return the Products to EnviroLogix for evaluation, EnviroLogix will repair or replace, at its option, any product or part thereof that proves defective in materials or workmanship within the warranty period.

ENVIROLOGIX MAKES NO OTHER WARRANTIES, EXPRESSED OR IMPLIED, INCLUDING BUT NOT LIMITED TO ANY IMPLIED WARRANTIES OF MERCHANTABILITY OR FITNESS FOR A PARTICULAR PURPOSE. The warranty provided herein and the data, specifications and descriptions of EnviroLogix products appearing in EnviroLogix published catalogues and product literature are EnviroLogix’ sole representations concerning the Products and warranty. No other statements or representations, written or oral, by EnviroLogix’ employees, agents or representatives, except written statements signed by a duly authorized officer of EnviroLogix Inc., are authorized; they should not be relied upon by the customer and are not a part of the contract of sale or of this warranty.

EnviroLogix does not warrant against damages or defects arising in shipping or handling, or out of accident or improper or abnormal use of the Products; against defects in products or components not manufactured by EnviroLogix, or against damages resulting from such non-EnviroLogix made products or components. EnviroLogix passes on to customer the warranty it received (if any) from the maker thereof of such non-EnviroLogix made products or components. This warranty also does not apply to Products to which changes or modifications have been made or attempted by persons other than pursuant to written authorization by EnviroLogix.

THIS WARRANTY IS EXCLUSIVE. The sole and exclusive obligation of EnviroLogix shall be to repair or replace the defective Products in the manner and for the period provided above. EnviroLogix shall not have any other obligation with respect to the Products or any part thereof, whether based on contract, tort, strict liability or otherwise. Under no circumstances, whether based on this Limited Warranty or otherwise, shall EnviroLogix be liable for incidental, special, or consequential damages.

This Limited Warranty states the entire obligation of EnviroLogix with respect to the Products. If any part of this Limited Warranty is determined to be void or illegal, the remainder shall remain in full force and effect.

*LibertyLink is a trademark of Bayer
EnviroLogix, the EnviroLogix logo, and QuickStix are trademarks of EnviroLogix Inc.*

© EnviroLogix 2006